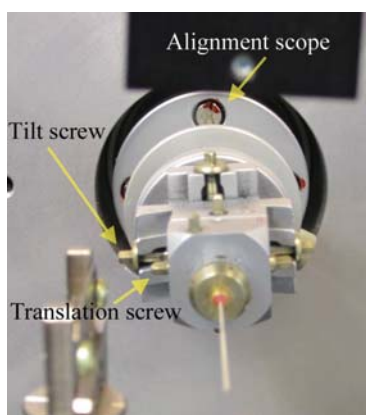


## 2. INSTRUMENTATION AND SAMPLE PREPARATION



**Figure 2.10.49**  
Goniometer head position in relation to the goniometer-mounted alignment scope.

movement rather than any wobble from tilt misalignment. However, it can still take some time. For systems where the goniometer spinning is controlled by computer software a wireless computer mouse is a very good investment, as it allows the person performing the alignment to stop the spinning capillary without taking their eyes off the sample.

### 2.10.2. Neutron powder diffraction

#### 2.10.2.1. Specimen form

Large penetration depth and sensitivity to lighter elements (especially mobile species such as hydrogen, lithium and oxygen) in the presence of heavier elements make neutron diffraction a powerful and complementary technique to X-ray diffraction for structural studies. Because neutrons are highly penetrating and large sample volumes can be used, sometimes no specimen preparation is needed at all; sintered ceramic pellets, fish otoliths and renal calculi can be placed directly in the beam. However, the most traditional sample holder for standard neutron powder diffraction (Debye–Scherrer geometry) is cylindrical and is usually made of vanadium. If the diffraction instrument has reflection geometry, however, one has to use flat plates. Diffractometers built for the study of engineering materials can accommodate various shapes and forms because they can isolate small volumes within the sample.

#### 2.10.2.2. Sample size

Traditionally, a large amount of sample was needed for neutron powder diffraction because of the limited flux available at various neutron sources. However, significant advances have been made in source power and detector technology, making it possible to do standard diffraction experiments with relatively small quantities of samples, both at reactor and spallation sources. There are multiple factors that have to be taken into account to determine how much sample is required. These include source power, detector coverage of the instrument, source-to-sample distance, the scattering power of the sample, beam size, available time and information sought from the measurement. Neutron powder diffraction instruments often have to trade intensity for resolution, and so often a larger quantity of sample is needed for high-resolution instruments. Sample mass can vary from milligrammes to several grammes, so it is always advisable to contact the scientists responsible for the particular instrument to determine the quantity needed for the proposed measurements.



(a)



(b)

**Figure 2.10.50**  
Two examples of sample holders used in neutron powder diffraction. (a) A cell made of Inconel used for hydrogen absorption studies in  $\text{Li}_3\text{N}$  (Huq *et al.*, 2007). (b) Vanadium holders that were specially made for a sample changer built for the Powgen diffractometer located at Oak Ridge National Laboratory.

#### 2.10.2.3. Specimen containment

The choice of materials for designing sample holders usually depends on the type of experiments, temperature or pressure conditions, the type of neutron source (constant-wavelength or time-of-flight), the presence or absence of fine radial collimators in the instrument and finally the sample. The scattering of vanadium ( $\sigma_{\text{coh}} = 0.0184 \text{ b}$ ) or a TiZr alloy (a null scatterer, because of exact matching of the negative scattering length of titanium and the positive scattering length of zirconium) is almost purely incoherent, making it ideal for sample containment for diffraction measurements. Although the coherent scattering of vanadium is small, in careful work it should not be a surprise to find weak peaks from V (space group  $Im\bar{3}m$ ,  $a = 3.027 \text{ \AA}$ ) in the powder pattern. Examples of vanadium sample cans are shown in Fig. 2.10.50(b). At a reactor source aluminium is even better if low-angle (large  $d$ -spacing) reflections are of interest, as in the case of many magnetic structural studies, because the aluminium incoherent scattering cross section is three orders of magnitude less than that of vanadium. At elevated temperatures, vanadium easily forms oxides or hydrides in the presence of air or hydrogen, making the cell brittle, so its use is limited to low-temperature studies or in vacuum furnaces. At temperatures higher than 1273 K one often has to use boron nitride caps and molybdenum screws for vanadium sample holders to avoid eutectic formation (an example is shown in Fig. 2.10.51b). For